

Report External Quality Control CoaguChek XS / XS Pro

Institution	ECAT Foundation
City	Voorschoten
Date of control	June 18, 2015
Monitor Serial no.	U812345
Strip Code	100
Batch no. QC set	B241B00.01



Test results

Sample	Target	%U ⁽¹⁾	Target Range	Measured	%D	Conclusion
1	2.1	0.8	1.8 - 2.4	1.9	-9.5	OK
2	2.7	0.6	2.3 - 3.1	2.8	3.7	OK
3	3.8	0.6	3.2 - 4.4	3.5	-7.9	OK
4	4.3	0.9	3.7 - 4.9	4.4	2.3	OK

1) Relative uncertainty of the target value

Evaluation

	Acceptance range	Measured	Conclusion
Correlation	0.950	0.963	OK
Slope	0.80 - 1.20	1.04	OK
Intercept	-0.50 - 0.50	-0.19	OK
Correct QC Results	4	4	OK

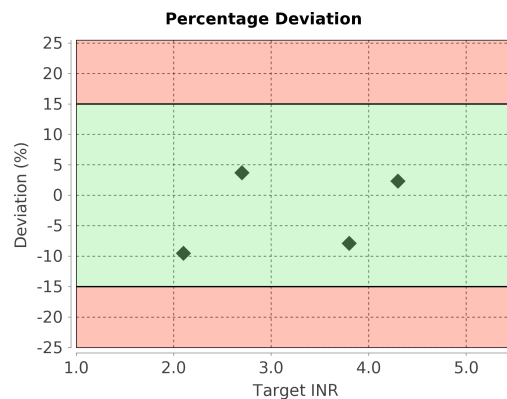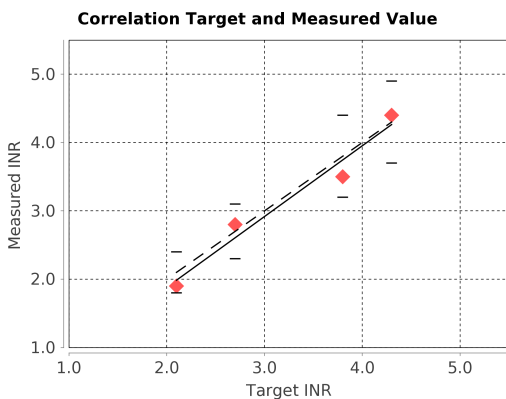

Final conclusion

This CoaguChek XS / XS Pro monitor passes the ECAT criteria for quality control:	YES
--	------------

Remarks

Signature + Date:



June 18, 2015

Dr. P. Meijer / Director ECAT Foundation